


PRODUCT DESCRIPTION

DigiL/E-xx probe with the I²C output is designed to measure air temperature and relative humidity in chemically non-aggressive environments. It is designed for connection to COMET devices equipped with inputs for Digi/E series probes. The probe is interchangeable, the calibration constants are saved in the internal memory of the probe. This probe **cannot** be connected to devices with analog inputs, for example a Pt1000 temperature probe.

The probes are supplied in several variants depending on the cable length (last two digits of the probe name indicate the cable length) and they are suitable for stationary or portable applications.

TECHNICAL PARAMETERS

- Temperature
 - Range: -30 to +105 °C
 - Accuracy: ± 0.4 °C
 - Response time: $t_{90} < 6$ min (temperature step 20 °C, air flow 1 m/s)
- Relative humidity
 - Range: 0 to 100 %RH (without condensation)
 - Accuracy of the humidity sensor: ± 1.8 %RH in the range of 0 to 90 %RH at 23 °C
 - Hysteresis: $< \pm 1$ %RH
 - Linearity error: $< \pm 1$ %RH
 - Temperature error: 0,05 % RH/°C (0 °C to +60 °C)
 - Response time: $t_{90} < 9$ s (humidity step 60 %RH, constant temperature)
- Calculated humidity quantities
 - 1/ Dew point temperature
 - Range: -60 to +80 °C
 - Accuracy:

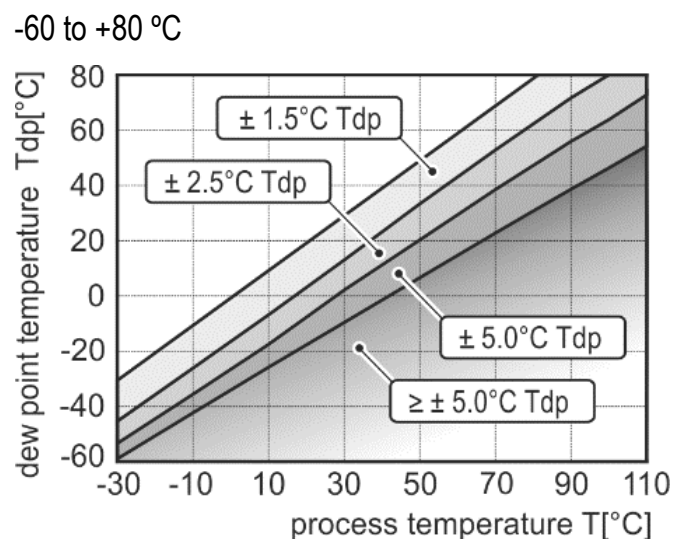

2/ Absolute humidity

Range: 0 to 400 g/m³

Accuracy: ±1.5 g/m³ for ambient temperature T < 25 °C

3/ Specific humidity

Range: 0 to 550 g/kg

Accuracy: ±2 g/kg for ambient temperature T < 35 °C and atmospheric pressure of 1013 hPa

4/ Mixing ratio

Range: 0 to 995 g/kg


Accuracy: ±2 g/kg for ambient temperature T < 35 °C and atmospheric pressure of 1013 hPa

5/ Specific enthalpy

Range: 0 to 995 kJ/kg


Accuracy: ±5 kJ/kg for ambient temperature T < 35 °C and atmospheric pressure of 1013 hPa

- Relative humidity and temperature restriction:

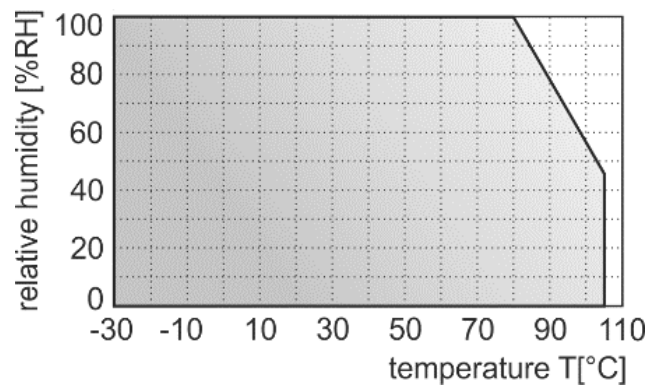

- Operating temperature range: -30 to +105 °C
- Operating relative humidity range: 0 to 100% RH (without condensation)
- Power: 2.7 to 5.5 V
- Current consumption: 50 µA @ 5 V
- Recommended calibration interval: 1 year
- Storage temperature: -10 to +60 °C
- Storage relative humidity: 0 to 100% RH (without condensation)
- Electromagnetic compatibility: EN 61326-1 (tested with device)
 - Emission: EN 55011, class B
 - Immunity: EN 61000-4-2, 4 kV/8 kV, class A
 - EN 61000-4-3, 3 V/m, class A
 - EN 61000-4-4, 0.5 kV/ 1 kV, class A
 - EN 61000-4-6, 3 V, class A
- Protection: IP40
- Filtering ability of the sensor cover: 0.025 mm
- Working position: without restriction
- Cable length: 1m, 2m, 5m, 10m, 15m
- Weight (with cable): 55g / 1m, 80g / 2m, 155g / 5m, 275g / 10m, 395g / 15m
- Material: ABS

DIMENSIONS

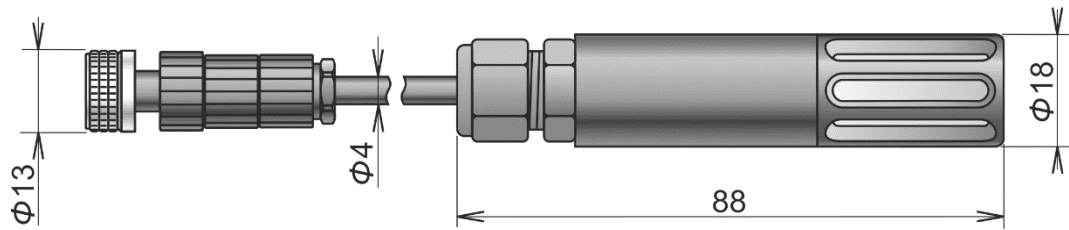

INSTALLATION

The probe place to area of measurement and connect it to the device.

For mounting of the probe it is possible to use the wall holder SP009 (optional accessories).

The probe does not require any special service or maintenance. We recommend you periodically to verify the accuracy of measurement by calibration.

TECHNICAL SUPPORT AND SERVICE

Technical support and service is provided by distributor. For contact see warranty certificate.

If needed, you can also use the discussion forum at <http://www.forum.cometsystem.cz/>.

WARNING



- It is not recommended to use the probe for long time under condensation conditions.
- Don't connect or disconnect the probe cable while the device is turned on - incorrect values could be recorded to the device memory.
- Don't use and don't store the probe without the sensor cover.
- The probe contains electronic components, it needs to liquidate them according to legal requirements.

Warranty certificate

This product has three years warranty since the date of sale to the end user. Defects due defective materials, defective manufacturing or design will be repaired free of charge by the manufacturer. The location of repair is at manufacturer's. No warranty is given to products operated in conditions not matching the conditions specified by the manufacturer in instruction manual. Also no warranty is given to products which were modified by the user, products with broken seal, products which were connected to power or input signals not matching the technical specification (Instruction manual). No warranty is given to consumables, e.g. batteries, fuses and eventual changes of parameters created by wear (influence of aggressive environment etc.).

Serial number:

Sale date:

DISTRIBUTOR

Accessory list

Instrument	Ordered	Shipped
DigiL/E-xx	✓	
SP009 - wall holder for external probes		
F5300 - PTFE sensor cover		

Completion verified by:

Date:

Signature: